

Diffuse reflectance spectroscopy to monitor murine colorectal tumor progression and therapeutic response (Erratum)

Ariel I. Mundo
Gage. J. Greening
Michael J. Fahr, Jr.
Lawrence N. Hale
Elizabeth A. Bullard
Narasimhan Rajaram
Timothy J. Muldoon

Diffuse reflectance spectroscopy to monitor murine colorectal tumor progression and therapeutic response (Erratum)

Ariel I. Mundo,^a Gage. J. Greening,^a Michael J. Fahr Jr.,^b
Lawrence N. Hale,^c Elizabeth A. Bullard,^a Narasimhan Rajaram,^a and
Timothy J. Muldoon^a

^aUniversity of Arkansas, Department of Biomedical Engineering, Fayetteville, Arkansas, United States

^bUniversity of Arkansas, Department of Computer Science, Fayetteville, Arkansas, United States


^cUniversity of Arkansas, Department of Chemistry and Biochemistry, Fayetteville, Arkansas, United States

[DOI: [10.1117/1.JBO.25.4.049803](https://doi.org/10.1117/1.JBO.25.4.049803)]


This article [*J. Biomed. Opt.* **25**(3), 035002 (2019) doi: [10.1117/1.JBO.25.3.035002](https://doi.org/10.1117/1.JBO.25.3.035002)] was originally published online on 6 March 2020 with an error in Figure 5, corresponding to percentage errors for the optical properties.

The article included a version of the figure that listed the wrong values. The text of Section 3.1 correctly states, “Average errors were 9.4 and 6.7 for μ'_s and μ_a , respectively [Figs. 5(a) and 5(b)]”; however, in Fig 5 the average errors were incorrectly listed as 6.9 and 5.0. The incorrect figure has been replaced with a corrected version.

Original figure:

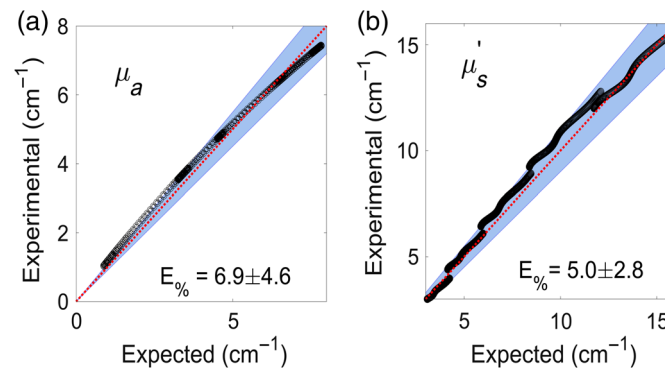

Corrected figure:

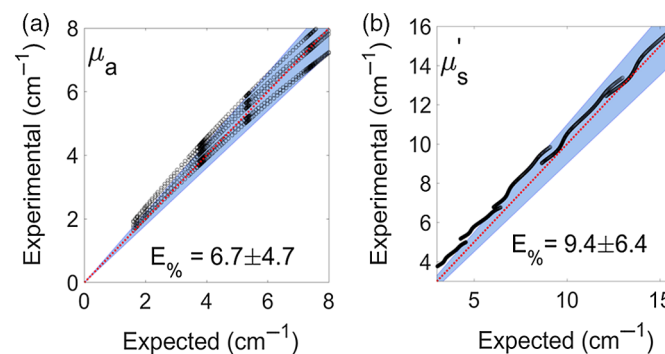

The caption for the figure is unchanged. The results reported were not affected by the error.

This article was corrected online on 27 March 2020.